

# COVID-19 FACE SHIELDS

**NOW AVAILABLE - 7-10 BUSINESS DAY DELIVERY**



QTY	1-50	51-150	151-499	500-999	1000+
EACH	\$19.25	\$18.25	\$14.95	\$12.95	\$10.95

- Following the protocol developed by the University of Wisconsin-Madison, Joseph Merritt & Company is manufacturing face shields as an emergency effort to provide PPE to those on the front lines during the COVID-19 crisis. The design for this mask has been approved and vetted by the infection control department at the UW Health University Hospital.

**FREE LOCAL DELIVERY TO CT AND RI  
WITH PURCHASE OF 500+**

**FULLY ASSEMBLED READY FOR USE:**

- **MEDICAL**
- **HEALTH CARE**
- **FOOD SERVICE**
- **GROCERY STORES**
- **FIRST RESPONDERS**

**ALL SALES FINAL • NO RETURNS**



Email: [info@josephmerritt.com](mailto:info@josephmerritt.com) or call our branches directly:

Hartford, CT (860)296-2500 • Danbury, CT (203)743-6734

New Haven, CT (203)562-9885 • Providence, RI (401)272-9060

[WWW.JOSEPHMERRITT.COM](http://WWW.JOSEPHMERRITT.COM)

**JOSEPH**

**Merritt**

**& COMPANY** *since 1908*

# MERRITT FACE SHIELDS

## VISOR

The visor is manufactured from clear film material such as Mylar or similar PET. The PET film is die cut to the UW design. As the supply chain for this material becomes strained, a combination of 5 mil and 7 mil thickness are used.



## BROW FOAM


The brow foam is manufactured from a general purpose open or closed cell foam with a pressure sensitive adhesive.

## ELASTIC HEADBAND

The elastic headband is manufactured from the widest range of materials.

Bulk suppliers for 1" braided elastic band are severely overwhelmed.

As such, our mask may be manufactured with the originally prescribed 1" elastic band, or a suitable replacement, such as a closed cell elastic silicon sponge banding, or a pair of elastic silicon cords.

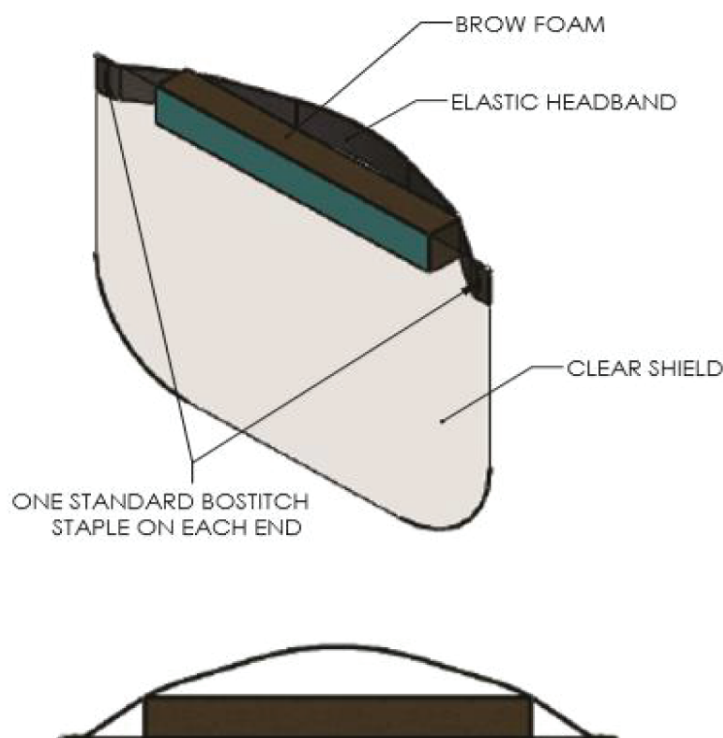

**DISCLAIMER AND WARRANTY:** This face shield is being provided to the wider community during this public health emergency. This product design has been approved and vetted by the infection control department at the UW Health University Hospital recommended for "one time use". However, this product has not been cleared for medical use by the U.S. Food and Drug Administration. This product has not been evaluated for the prevention of specific diseases or infections, the filtering of surgical smoke or plumes, the filtering of specific amounts of viruses or bacteria, or the killing or reduction of the amount of viruses, bacteria, or fungi. Individuals or organizations using this product are responsible for informing healthcare providers and end users, to which the masks are supplied that they are responsible for decisions regarding appropriate Personal Protective Equipment (PPE) for their personnel and/or individual use. No warranties of any kind are offered for the face shield design and specifications, including warranties of non-independent and fitness for a particular purpose.

Email: [info@josephmerritt.com](mailto:info@josephmerritt.com) or call our branches directly:

Hartford, CT (860)296-2500 • Danbury, CT (203)743-6734

New Haven, CT (203)562-9885 • Providence, RI (401)272-9060

JOSEPH

**Merritt**

& COMPANY since 1908

[WWW.JOSEPHMERRITT.COM](http://WWW.JOSEPHMERRITT.COM)